

Molecularly Imprinted Polymers for the Capacitive Detection of Amphetamine-Type Stimulants

Suzan El-Akaad¹, Michael Pütz², Martin Hedström³, Sarah De Saeger¹, and Natalia Beloglazova¹

¹Centre of Excellence in Mycotoxigenology and Public Health, Ghent University, Ottergemsesteenweg 460, B-9000 Ghent, Belgium


²Bundeskriminalamt, Forensic Science Institute, KT45 – Toxicology, 65173 Wiesbaden Germany

³Capsenze HB, Medicon Village, SE-22381 Lund, Sweden


Introduction

- Illicit drug use includes the non-medical use of a variety of drugs that are prohibited by international law.
- Detection of chemical markers related to the illegal synthesis of these drugs of abuse in sewage water is an approach to monitor the imperilment of the environment by chemical production waste.
- This work presents a capacitive biosensor for the detection of 4 methyl- 5 phenylpyrimidine (4M5PP) as an ATS-marker using molecularly imprinted polymers (MIP) as recognition elements.


Materials & Methods

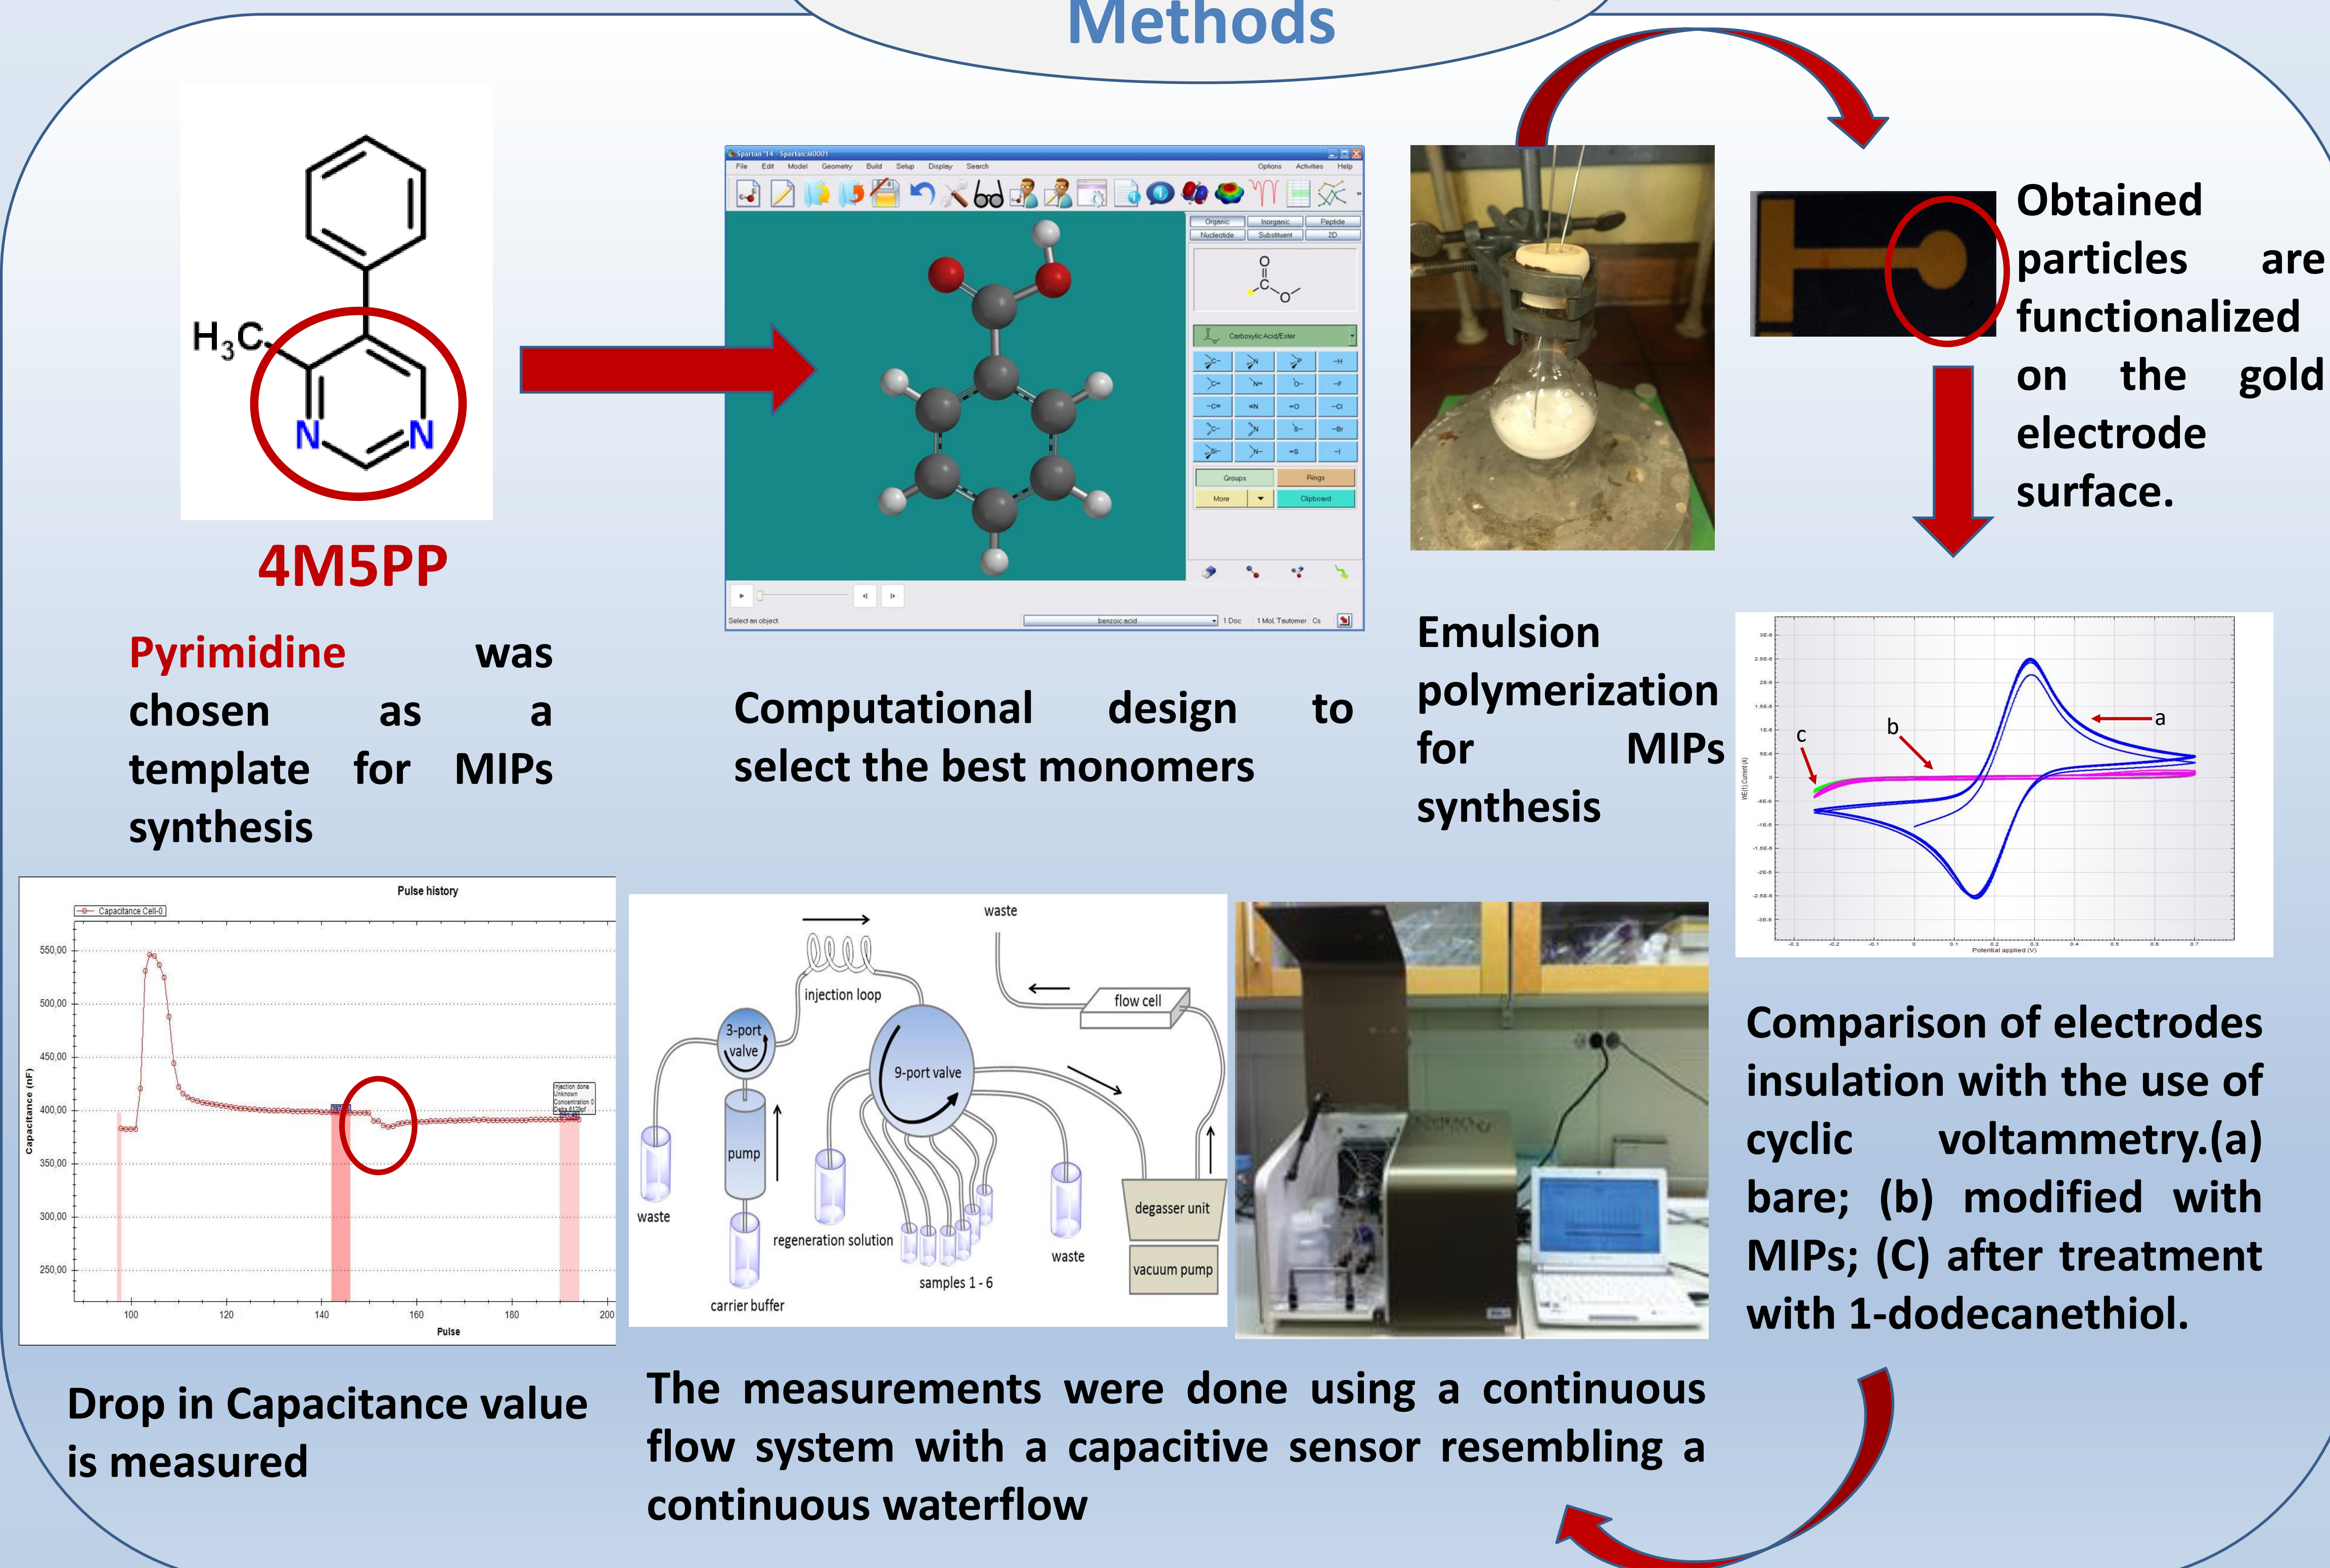


Results & Discussion

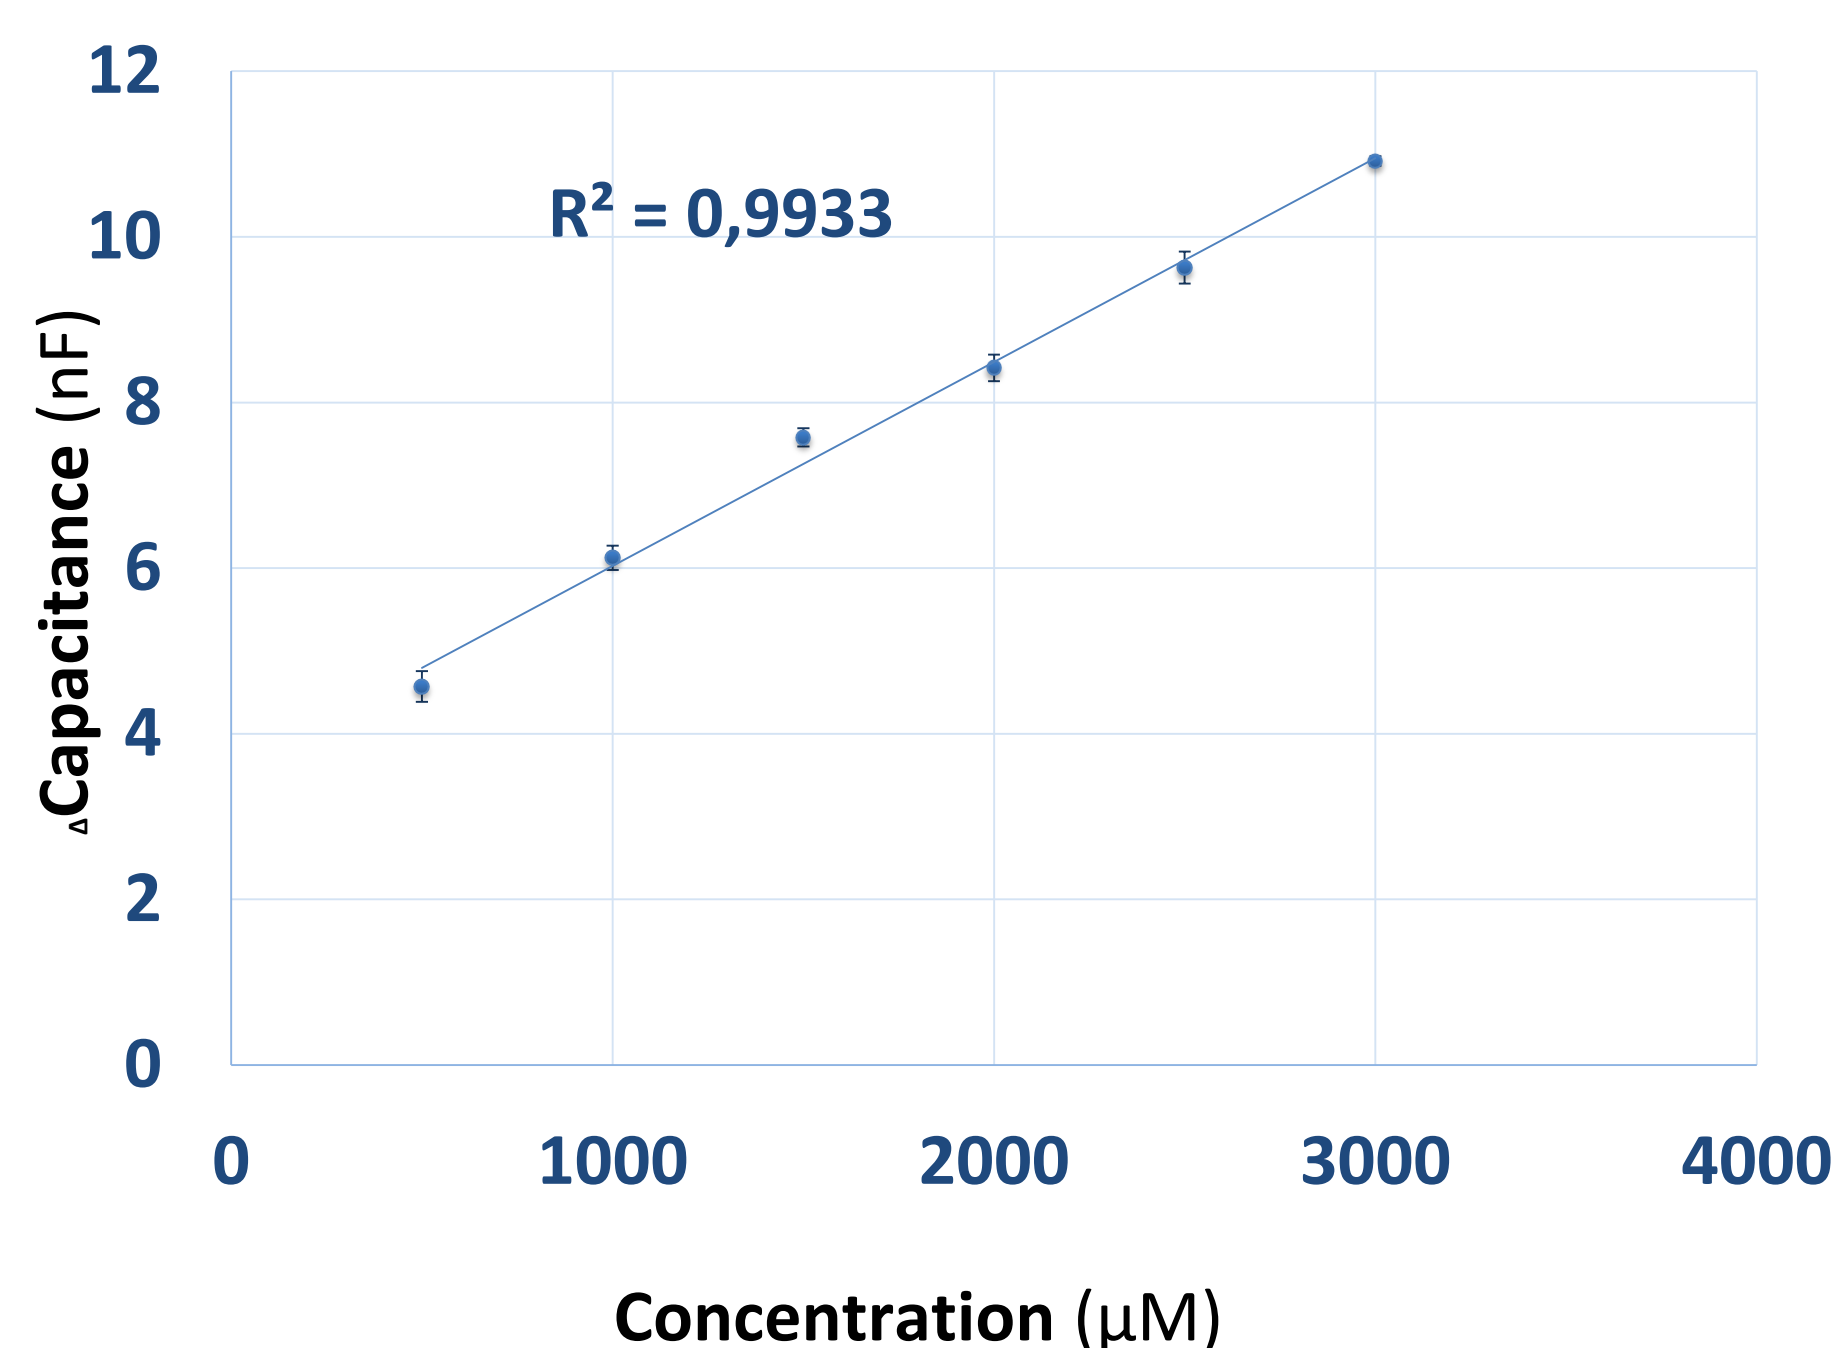

Change in capacitance (nF) of the MIP functionalized electrode as a function of concentration (μM). The limit of detection is $500 \mu\text{M}$ with a linear range of $500 \mu\text{M} - 3 \text{ mM}$. The sensor was tested in environmental water samples, and it showed the same results as in purified water.

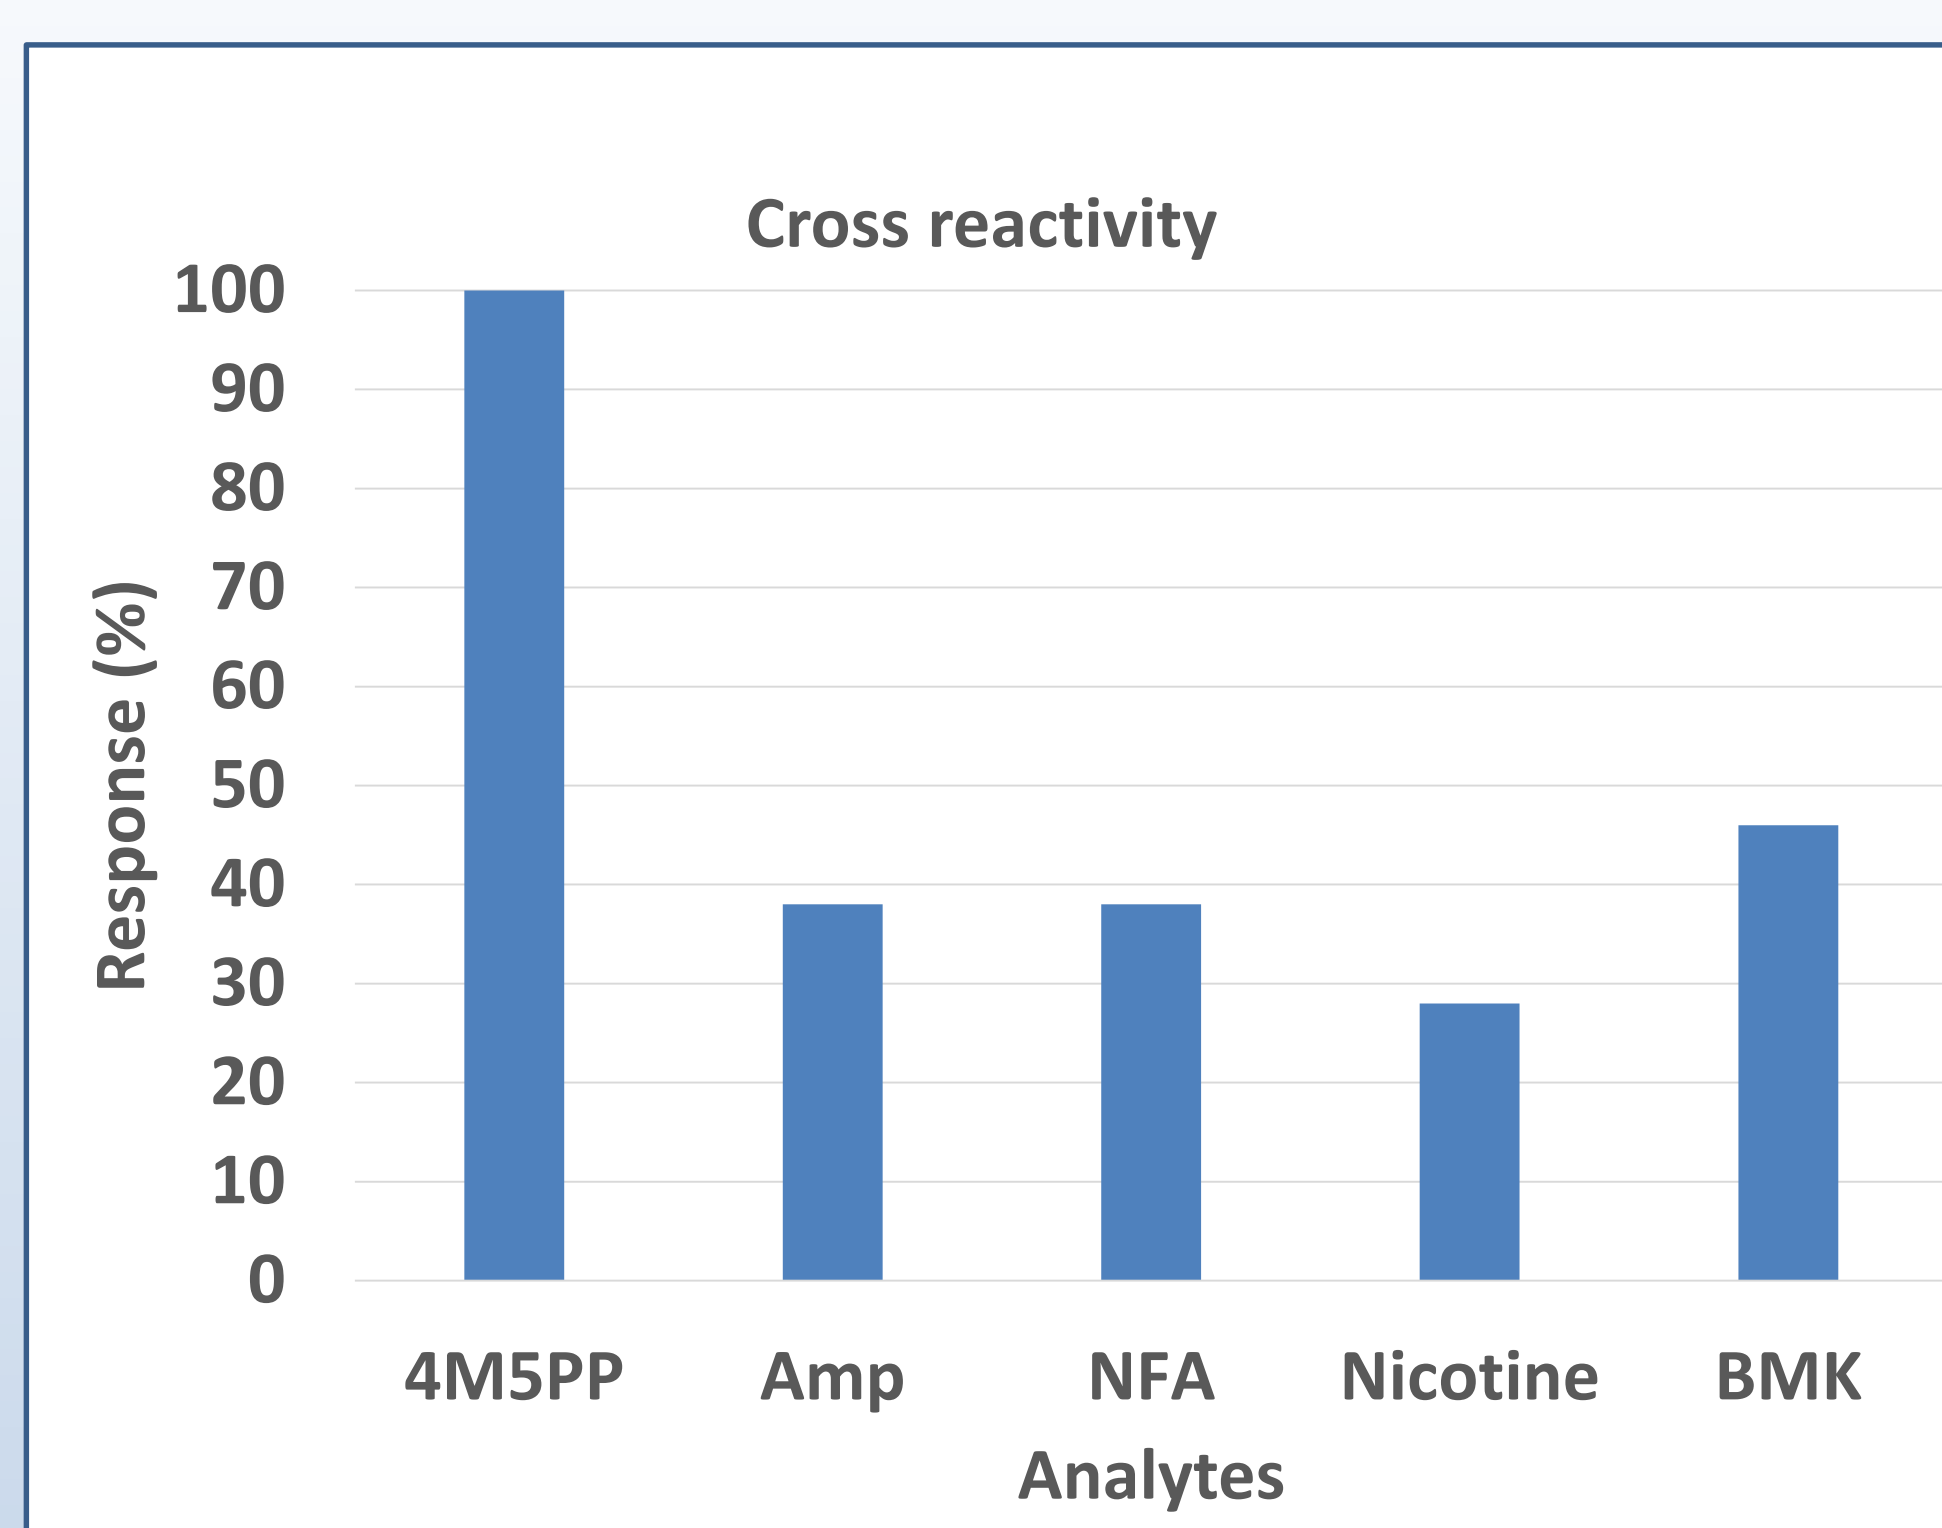

Cross-reactivity experiments performed with four structural similar compounds.

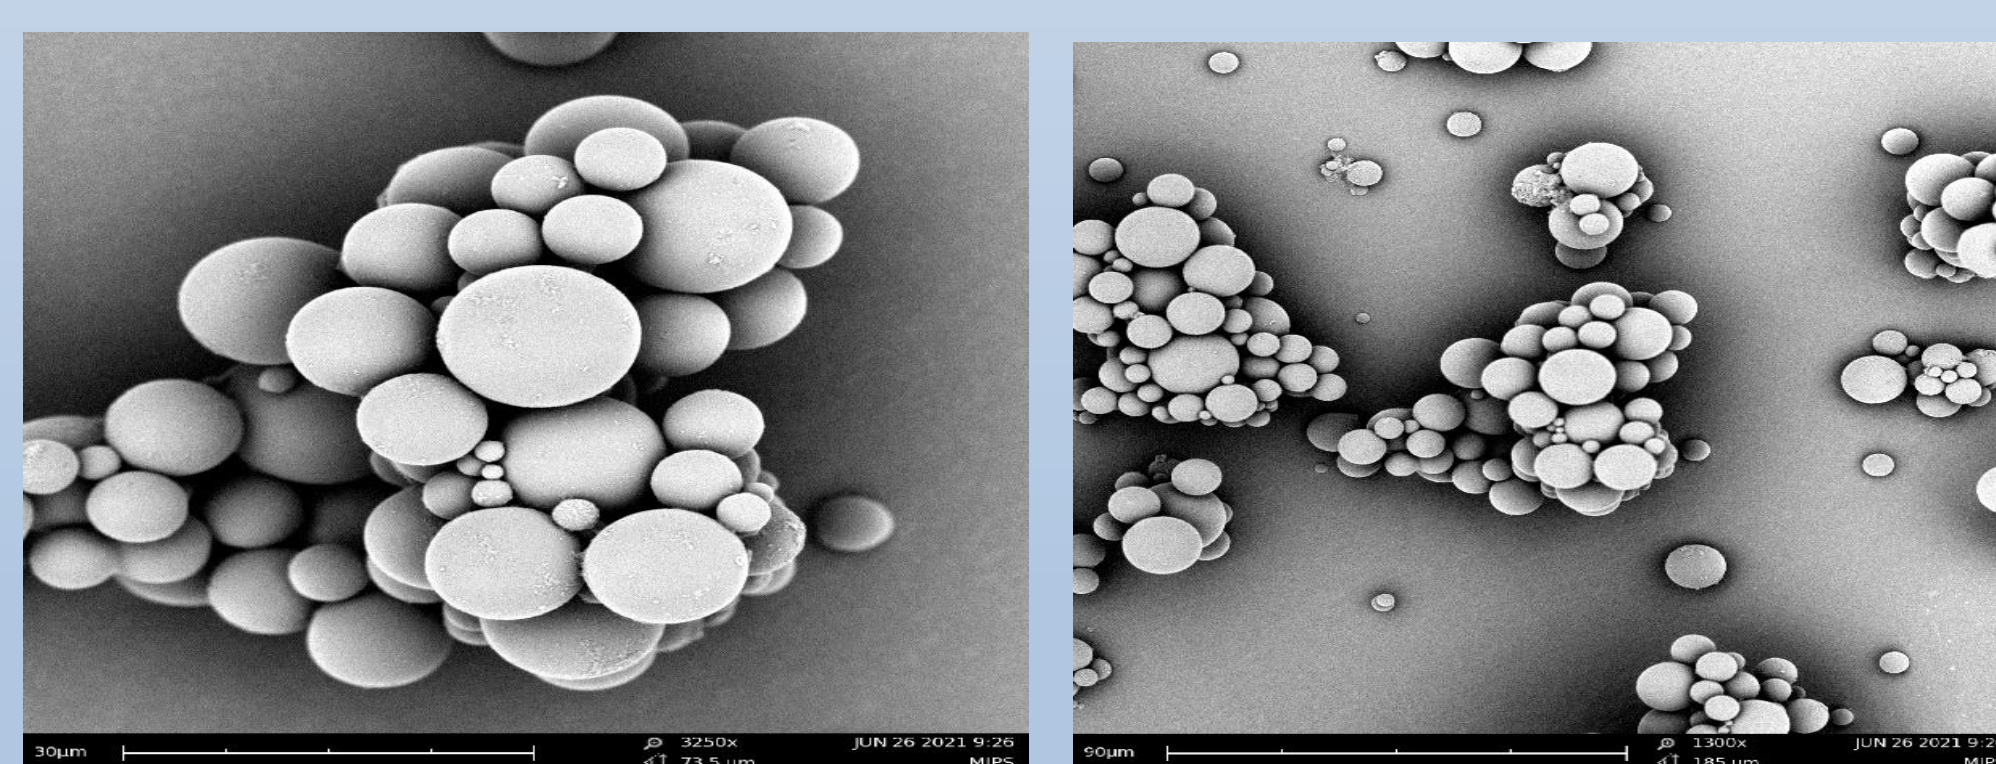

Scanning Electron Microscopy (SEM) pictures of synthesized molecularly imprinted polymers (MIPs), MIPs for 4M5PP prepared using emulsion polymerization.

Effect of Additives:

The impact of different additives on the capacitive signal (detergents, shampoos, pharmaceuticals, and sweeteners) was tested. Pharmaceuticals and sweeteners showed a decrease in the capacitance drop. The major impact resulted from the detergents and shampoo, with 0.1% detergent and 0.1% shampoo giving false positive results.

Conclusion

- The synthesized particles for 4M5PP showed high selectivity and significant sensitivity towards the target compound.
- The limit of detection was $500 \mu\text{M}$ with a linear range of $500 \mu\text{M} - 3 \text{ mM}$.
- The sensor could be used with real environmental water samples.

Corresponding author : beloglazovanv@gmail.com, natalia.beloglazova@gmail.com (N.V. Beloglazova)